

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
8 April 2004 (08.04.2004)

PCT

(10) International Publication Number
WO 2004/029851 A1

(51) International Patent Classification⁷: **G06F 19/00**

(21) International Application Number:
PCT/CA2003/001391

(22) International Filing Date:
24 September 2003 (24.09.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/413,055 24 September 2002 (24.09.2002) US

(71) Applicant (for all designated States except US): **EAST-MAN KODAK COMPANY** [US/US]; 343 State Street, Rochester, NY 14650-2201 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **MENHARDT, Wido** [CA/US]; 17706 Blackberry Hill, Los Gatos, CA


95030 (US). **ZHANG, Heidi** [CA/US]; 367 Penn Way, Los Gatos, CA 95032 (US). **HARRINGTON, Scott** [US/US]; 102 Hoskins Court, Unit #6F, Stanford, CA 94305 (US).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: METHOD AND SYSTEM FOR COMPUTER AIDED DETECTION (CAD) CUED READING OF MEDICAL IMAGES

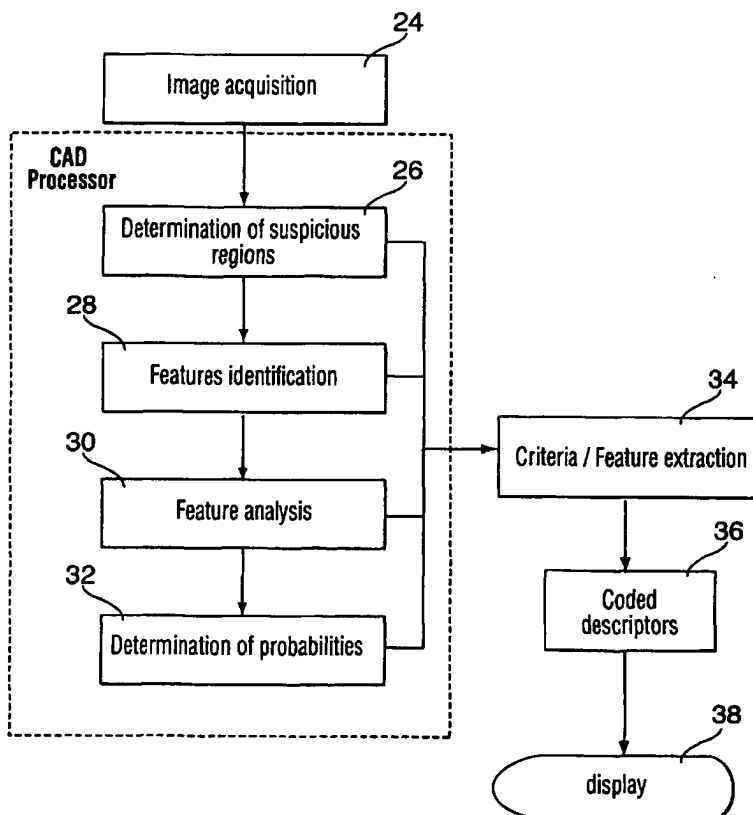

(57) Abstract: A method and system for Computer Aided Detection (CAD) of abnormalities in X-ray images in which the features and/or criteria used in the CAD analysis are displayed as coded descriptors on the digital image of the X-ray to provide an indication to a user of the basis underlying the identification of a particular abnormality therefore increasing the reliability of a diagnosis established by the user.